



BIOLOX CONTOURA®

Inspired by
Anatomy

BIOLOX®
MATERIAL
MATTERS®

ANATOMICALLY CONTOURED HEAD FOR TOTAL HIP ARTHROPLASTY

THA aims to restore the natural function of the hip by replacing the diseased joint with an artificial implant. BIOLOX CONTOURA® is a contoured femoral ceramic head mimicking the anatomical shape of the proximal femur. BIOLOX CONTOURA® was cleared for use in the USA by the FDA in August 2019.

It was conceived and developed at the Harris Orthopaedics Laboratory at Massachusetts General Hospital in Boston (MA, USA), by Drs. Orhun Muratoglu, Andrew Freiberg, Kartik M. Varadarajan, Harry Rubash and Henrik Malchau, and in cooperation with CeramTec GmbH.



It is just that we have come to assume that the femoral head should look like a sphere, but the truth is that it does not exactly reflect what the native hip looks like.

Orhun Muratoglu

1

Smooth transition

BIOLOX CONTOURA® femoral heads retain the outer diameter profile of conventional implants and incorporate a contoured shoulder with a lesser radius; a design conceived with the goal of reducing the volume of material potentially exposed to the soft tissue. The contoured design provides a smooth transition throughout the femoral head and the head-neck junction.

2

Material

Made of the proven material BIOLOX®*delta*, with excellent biocompatibility, low immunological response, high wear resistance and reduced bacterial adhesion.

BIOLOX CONTOURA®

Inspired by
Anatomy

BIOLOX®
MATERIAL
MATTERS®


CURRENT PORTFOLIO

28, 32, 36, 40, 44 mm

Multiple Neck Lengths: S, M, L, XL

32-12/14 M
Conventional head

36-12/14 M
BIOLOX CONTOURA®

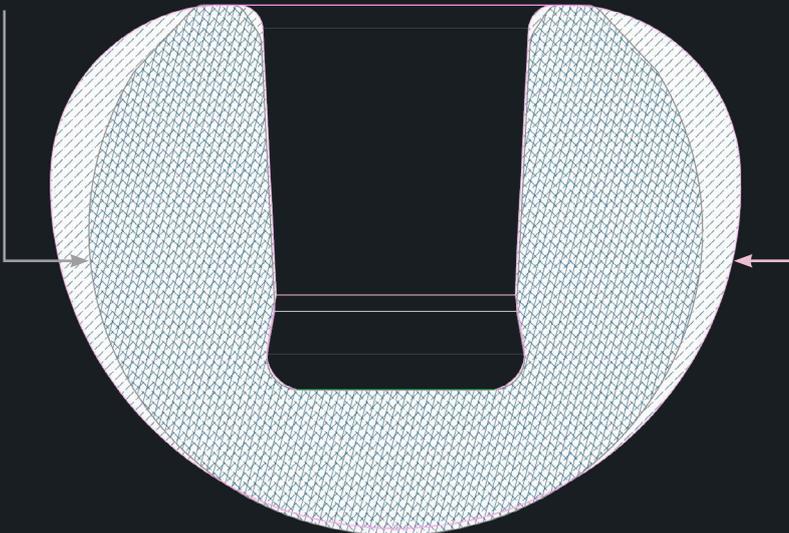

References

Faye PA, Roualides O, Rossignol F, Hartmann DJ, Desmoulière A. Engulfment of ceramic particles by fibroblasts does not alter cell behavior. *Biomed Mater*. 2017;12(1):015023. doi:10.1088/1748-605X/aa5aa2.

Cunningham BW, Hallab NJ, Hu N, McAfee PC. Epidural application of spinal instrumentation particulate wear debris: a comprehensive evaluation of neurotoxicity using an in vivo animal model. *J Neurosurg Spine*. 2013;19(3):336-350. doi:10.3171/2013.5.SPINE13166.

Savarino L, Baldini N, Ciapetti G, Pellacani A, Giunti A. Is wear debris responsible for failure in alumina-on-alumina implants? *Acta Orthop*. 2009;80(2):162-167. doi:10.3109/17453670902876730.

Asif IM, Williams S, Fisher J, Al-Hajjar M, Anderson J, Tipper JL. Characterisation and biocompatibility of composite ceramic particles used to manufacture ceramic-on-ceramic total hip replacements. *Front Bioeng Biotechnol*. 2016;00793. doi:10.3389/conf.FBIOE.2016.01.00793.

Asif I M. *Characterisation and Biological Impact of Wear Particles from Composite Ceramic Hip Replacements*. [PhD thesis]. Leeds, UK: University of Leeds; 2018. <http://etheses.whiterose.ac.uk/20563/>.

Krenn V, Thomsen P, Thomsen M, et al. Histopathological Particle Identification (The Krenn Particle Algorithm). *CeraNews*. 2013;2:12-17.

Grupp TM, Holderied M, Mulliez MA, et al. Biotribology of a vitamin E-stabilized polyethylene for hip arthroplasty – Influence of artificial ageing and third-body particles on wear. *Acta Biomater*. 2014;10:3068-3078. doi:10.1016/j.actbio.2014.02.052.

Nikolaou VS, Edwards MR, Bogoch E, Schemitsch EH, Waddell JP. A prospective randomized controlled trial comparing three alternative bearing surfaces in primary total hip replacement. *J Bone Joint Surg Br*. 2012;94-B(4):459-465. doi:10.1302/0301-620X.94B4.27735.

Piconi C, Porporati AA, Streicher RM. Ceramics in THR Bearings: Behavior under Off-Normal Conditions. *Key Engineering Materials*. 2014;631:3-7. doi:10.4028/www.scientific.net/kem.631.3.

Trampuz A, Maiolo EM, Winkler T, Perka C. Biofilm formation on ceramic, metal and

polyethylene bearing components from hip joint replacement systems. *Orthopaedic Proceedings*. 2016;98-B(SUPP 10):80-80. doi:10.1302/1358-992X.98BSUPP_10.ISTA2015-080.

Sorrentino R, Cochis A, Azzimonti B, et al. Reduced bacterial adhesion on ceramics used for arthroplasty applications. *J Eur Ceram Soc*. 2018;38(3):963-970. doi:10.1016/j.jeurceramsoc.2017.10.008.

Trampuz A, Maiolo EM, Winkler T, Perka C. Biofilm formation on ceramic, metal and polyethylene bearing components from hip joint replacement systems. *Orthopaedic Proceedings*. 2016;98-B(SUPP 10):80-80. doi:10.1302/1358-992X.98BSUPP_10.ISTA2015-080.

Sorrentino R, Cochis A, Azzimonti B, et al. Reduced bacterial adhesion on ceramics used for arthroplasty applications. *J Eur Ceram Soc*. 2018;38(3):963-970. doi:10.1016/j.jeurceramsoc.2017.10.008.

Varadarajan KM, Zumbunn T, Duffy MP, et al. Next Generation Soft-Tissue Friendly Large Diameter Femoral Head. *Seminars in Arthrop*. 2013;24(4):211-217. doi:10.1053/j.sart.2014.01.007.

Zumbunn T, Duffy MP, Varadarajan KM, et al. Contoura: A New Anatomically Contoured Femoral Head. *CeraNews*. 2014;2:10-11.

Varadarajan KM, Zumbunn T, Duffy MP, et al. Anatomically Contoured Large Diameter Heads Can Reduce Iliopsoas Impingement: A Cadaver Verification Study. *Seminars in Arthrop*. 2015;26(1):28-33. doi:10.1053/j.sart.2015.04.006.

Duffy MP, Varadarajan KM, Chan D, et al. Anatomical Contouring of Large Diameter Heads for Soft-tissue Relief Does Not Alter Load Bearing Contact Area and Wear Performance in Ceramic on Poly Articulation. *ORS website*. <http://www.ors.org/Transactions/60/1141.pdf>. Accessed March 06, 2020.

Varadarajan KM, Duffy MP, Zumbunn T, et al. A New Soft Tissue Friendly Femoral Head may also Reduce Frictional Torque in Ceramic-on-Ceramic Articulation. *ORS website*. <http://www.ors.org/Transactions/60/0921.pdf>. Accessed March 06, 2020.

